

Double Strand DNA Fragmentation Test Report

I. Sample Information

Patient ID: (None)

Sample ID: R11+ 15_0930_100



Abstinence Days : (None)

Sample Type : (None)

Collection Difficulties : (None)

Collected : (None)

Complete Sample : (None)


Received : (None)

Collection Method : (None)


Analysis Time : 2025/10/01 01:57

II. Double Strand DNA Fragmentation Analysis


Well 1	Count	%
- Normal	238	26.86
- Fragmented	648	73.14
Detail Classification		
- Halo	648	73.14
- No Halo	238	26.86
Total	886	100.00

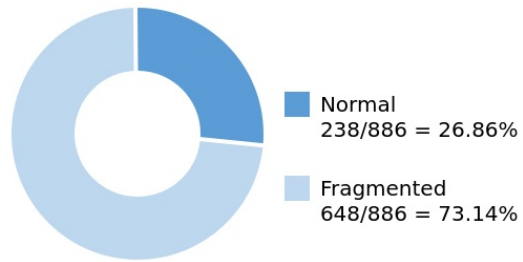


Well 2	Count	%
- Normal	544	73.41
- Fragmented	197	26.59
Detail Classification		
- Halo	197	26.59
- No Halo	544	73.41
Total	741	100.00

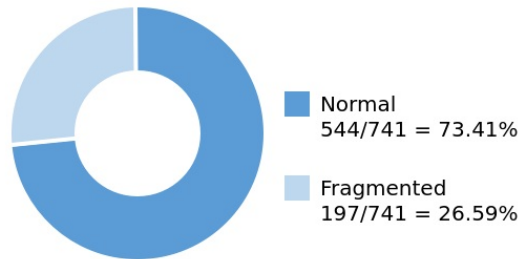

III. Result

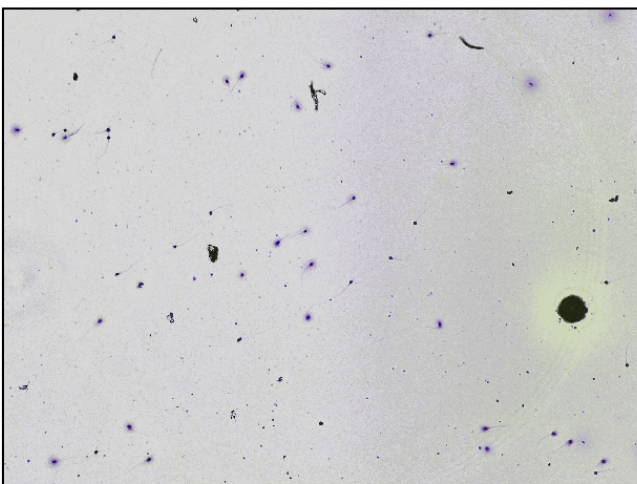

Sample Result	Count	%
- Normal	782	48.06
- Fragmented	845	51.94
Total	1627	100.00

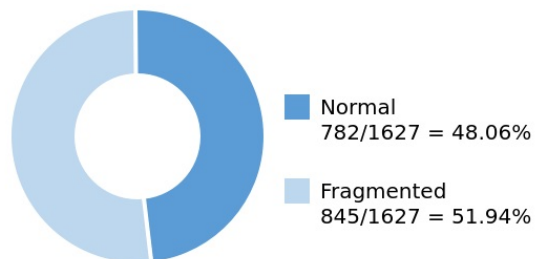

IV. Remark

Report Time : _____ Medical Technologist: _____ Supervisor: _____

Note : This report is only responsible for the specimens tested, only for clinical reference, no medical certificate.

Serial Number: X12YH18M10005; Software Version: X12.C04; Test Cassette: R11 Plus; Test Code: 10